


Yashraj Biotechnology Limited Real Time Real Temperature Stability Chart

Alpha 1 Microglobulin

Batch No.	Values of A1M on each testing in mg/ml by ELISA					
	07-01-09	09-03-09	08-04-09	22-06-09	22-07-09	20-08-09
BAM0001/09	2.79	2.83	2.82	2.85	2.80	2.75
BAM0002/09	2.79	2.79	2.81	2.93	2.91	2.90
BAM0003/09	2.91	-	2.99	2.96	2.94	2.92

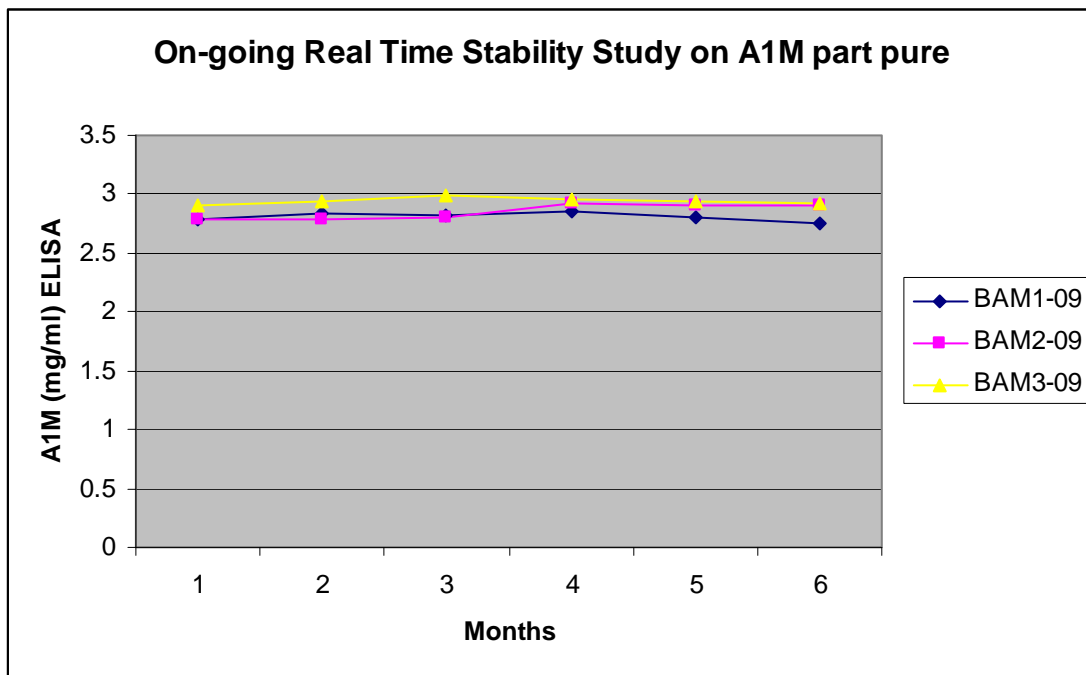

Opinion : A1M indicates good stability in values at 2-8°C and the study continues

Dr. Sanjeev Kumar Gupta, Manager QA/RA